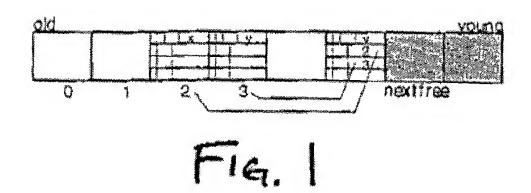
1/2 Janssen YOR920010266US1US2 (PJO)



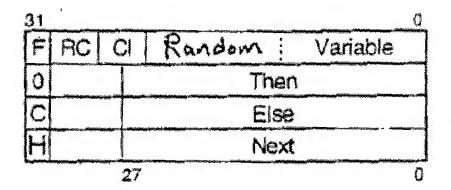


Fig. 2

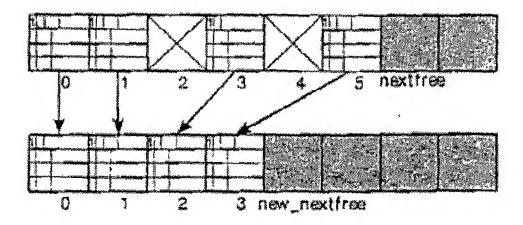
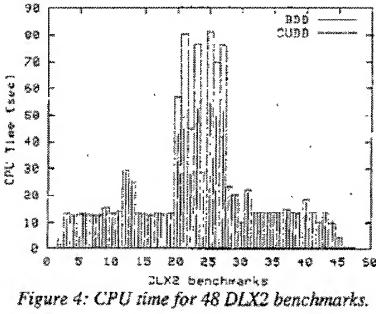
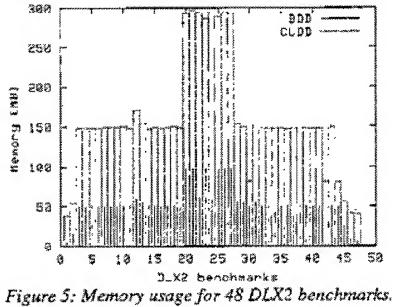


Fig. 3

2/2 Janssen YOR920010266US1US2 (PJO)





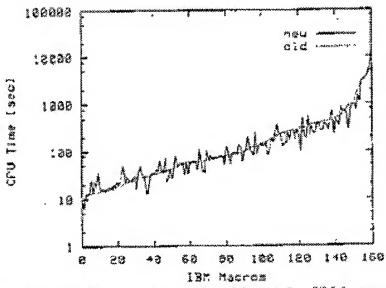


Figure 6: CPU time of new vs. old tool for IBM macros.